



Hydraulic Lifts & Slings

Model #: _____

Provider Name: _____

Serial #: _____

Phone #: _____

Date: _____

Contact Person: _____

Setting up your equipment:

- Place upper section in base taking care to be sure that it is locked in.
- Attach hanger on the end of the boom (arm).
- Attach sling to hanger according to manufacturer's instructions.
- Remember, while bringing through a home be careful to not damage doorways or walls, and also, lift with your legs, not your back.

Using your equipment:

- Before lifting patient, spread base legs fully outward with lever next to mast.
- Adjust sling straps or chains to proper height.
- Slide into position near patient being careful of swinging hanger.
- Once patient is in sling, lift just enough to clear surface & allow swivel.

To accommodate sling to patient: (Patient lying down)

- Roll patient away from you.
- Lay sling (patient side up) on surface where patient was lying.
- Adjust position of sling to line up with patient's buttocks and torso.
- Roll patient back to lying position over sling.
- Roll lift into place, and then lower boom to attach straps or chains to sling.

Frequent replacement items:

- Sling may need to be replaced after extensive use.

Maintenance:

- Cleaning of sling and double-checking of chains is recommended.
- Wash slings per manufacturer's instructions.

Diagram 1


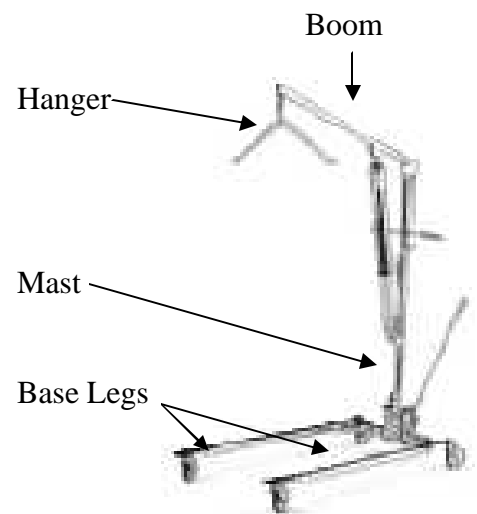


Diagram 2

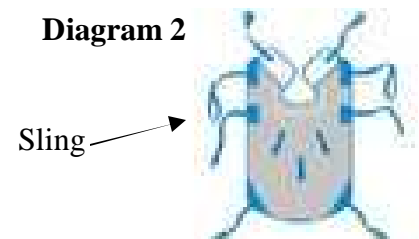

Special Procedures:

- Lifting from a seated position
 - Stand in front of a chair facing the patient.
 - Lean patient forward so your body supports their weight.
 - Hold sling by top. Allow remainder of sling material to drop behind patient to the seat of the chair.
 - To position the sling material under the patient's buttocks;
 - Lean patient to one side.
 - Reach underneath the patient's raised buttocks.
 - Firmly grasp sling material and pull toward patient's leg.
 - Repeat for other leg by switching the patient to lean in the opposite direction.
 - Once sling is properly positioned, roll lift into position and attach chains or straps.

- Lifting from floor
 - Repeat as for patient lying in bed.
 - Lower lift boom to lowest position to attach chains/straps to sling.
 - Follow lifting instructions above.

Safety Issues:

- Before use
 - Make sure patient's head is clear of hanger at all times.
 - Only raise boom high enough for patient in sling to clear the "transfer from" surface.
 - Make sure all parts of lift are properly secured.
 - Adjust chains or straps and sling prior to allowing patient to be lifted.
 - Spread legs of lift base to ensure maximum stability.
- When raising patient weight
 - Ensure that release is locked into "lift" position.
 - Check for pinch points on patient where the sling makes weight-bearing contact. Do this before rolling the lift away from the "transfer from" surface.
 - When moving lift (occupied) push slowly and smoothly towards "transfer to" surface.

Please contact your equipment provider for any questions, adjustments, or repairs.

Your local provider:



©Copyright The VGM Group
B.L.U.E. Sheet images, drawings, and text
courtesy of VGM contracted vendors.

All Medicare DMEPOS suppliers must be in compliance with CMS Supplier Standards in order to obtain and retain their billing privileges. These standards, in their entirety, are listed in 42 C.F.R. pt. 424, sec 424.57(c). A supplier must disclose these standards to all customers/patients who are Medicare beneficiaries (standard 16). Supplier Standard 12 includes "A supplier ...must instruct beneficiaries on use of Medicare covered items".